


# Volume Change Apparatus

ZI 1020

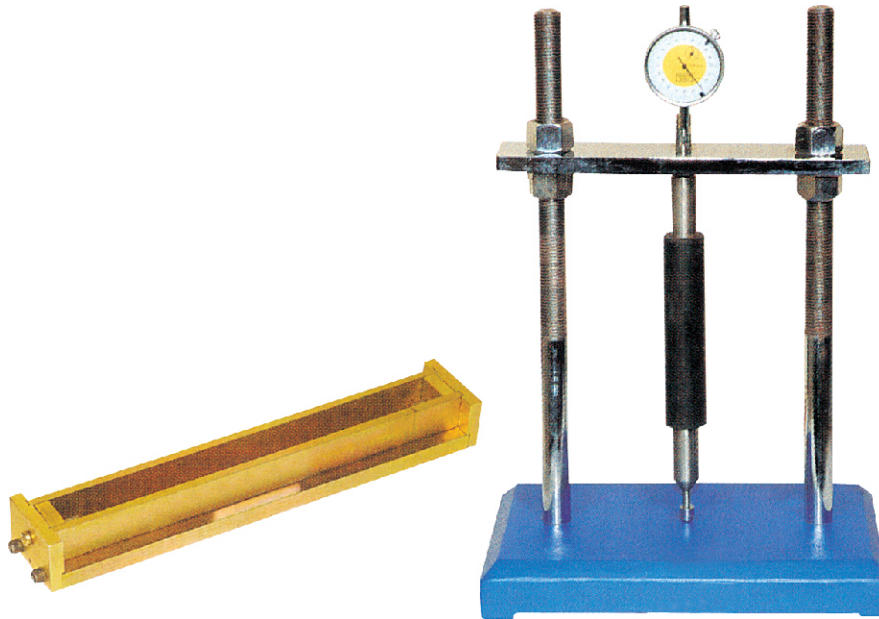

## Volume Change Apparatus : ZI 1020

ASTM C 490, IS 4031 & BS 1881.

The instrument is used for determining the volume change of cement concrete.

### SPECIFICATION :

The apparatus comprises of one mould effective gauge length complete with base plate, four reference pins, one length comparator frame, one stainless reference bar with insulated grip, and one dial gauge, 0.002mm x 10mm

## **ZEAL INTERNATIONAL**

1, Netaji Subhash Marg, Darya Ganj, New Delhi-110 002 INDIA  
Ph.:+91-11-23276114, 23244474, 23277528, 23278846, Fax :+91-11-23273214, 43580558  
E-mail : sales@zealinternational.com ,website : zealinternational.com